File Pre Guide For 47.25″ x 118.125″ EMS XLarge Banner

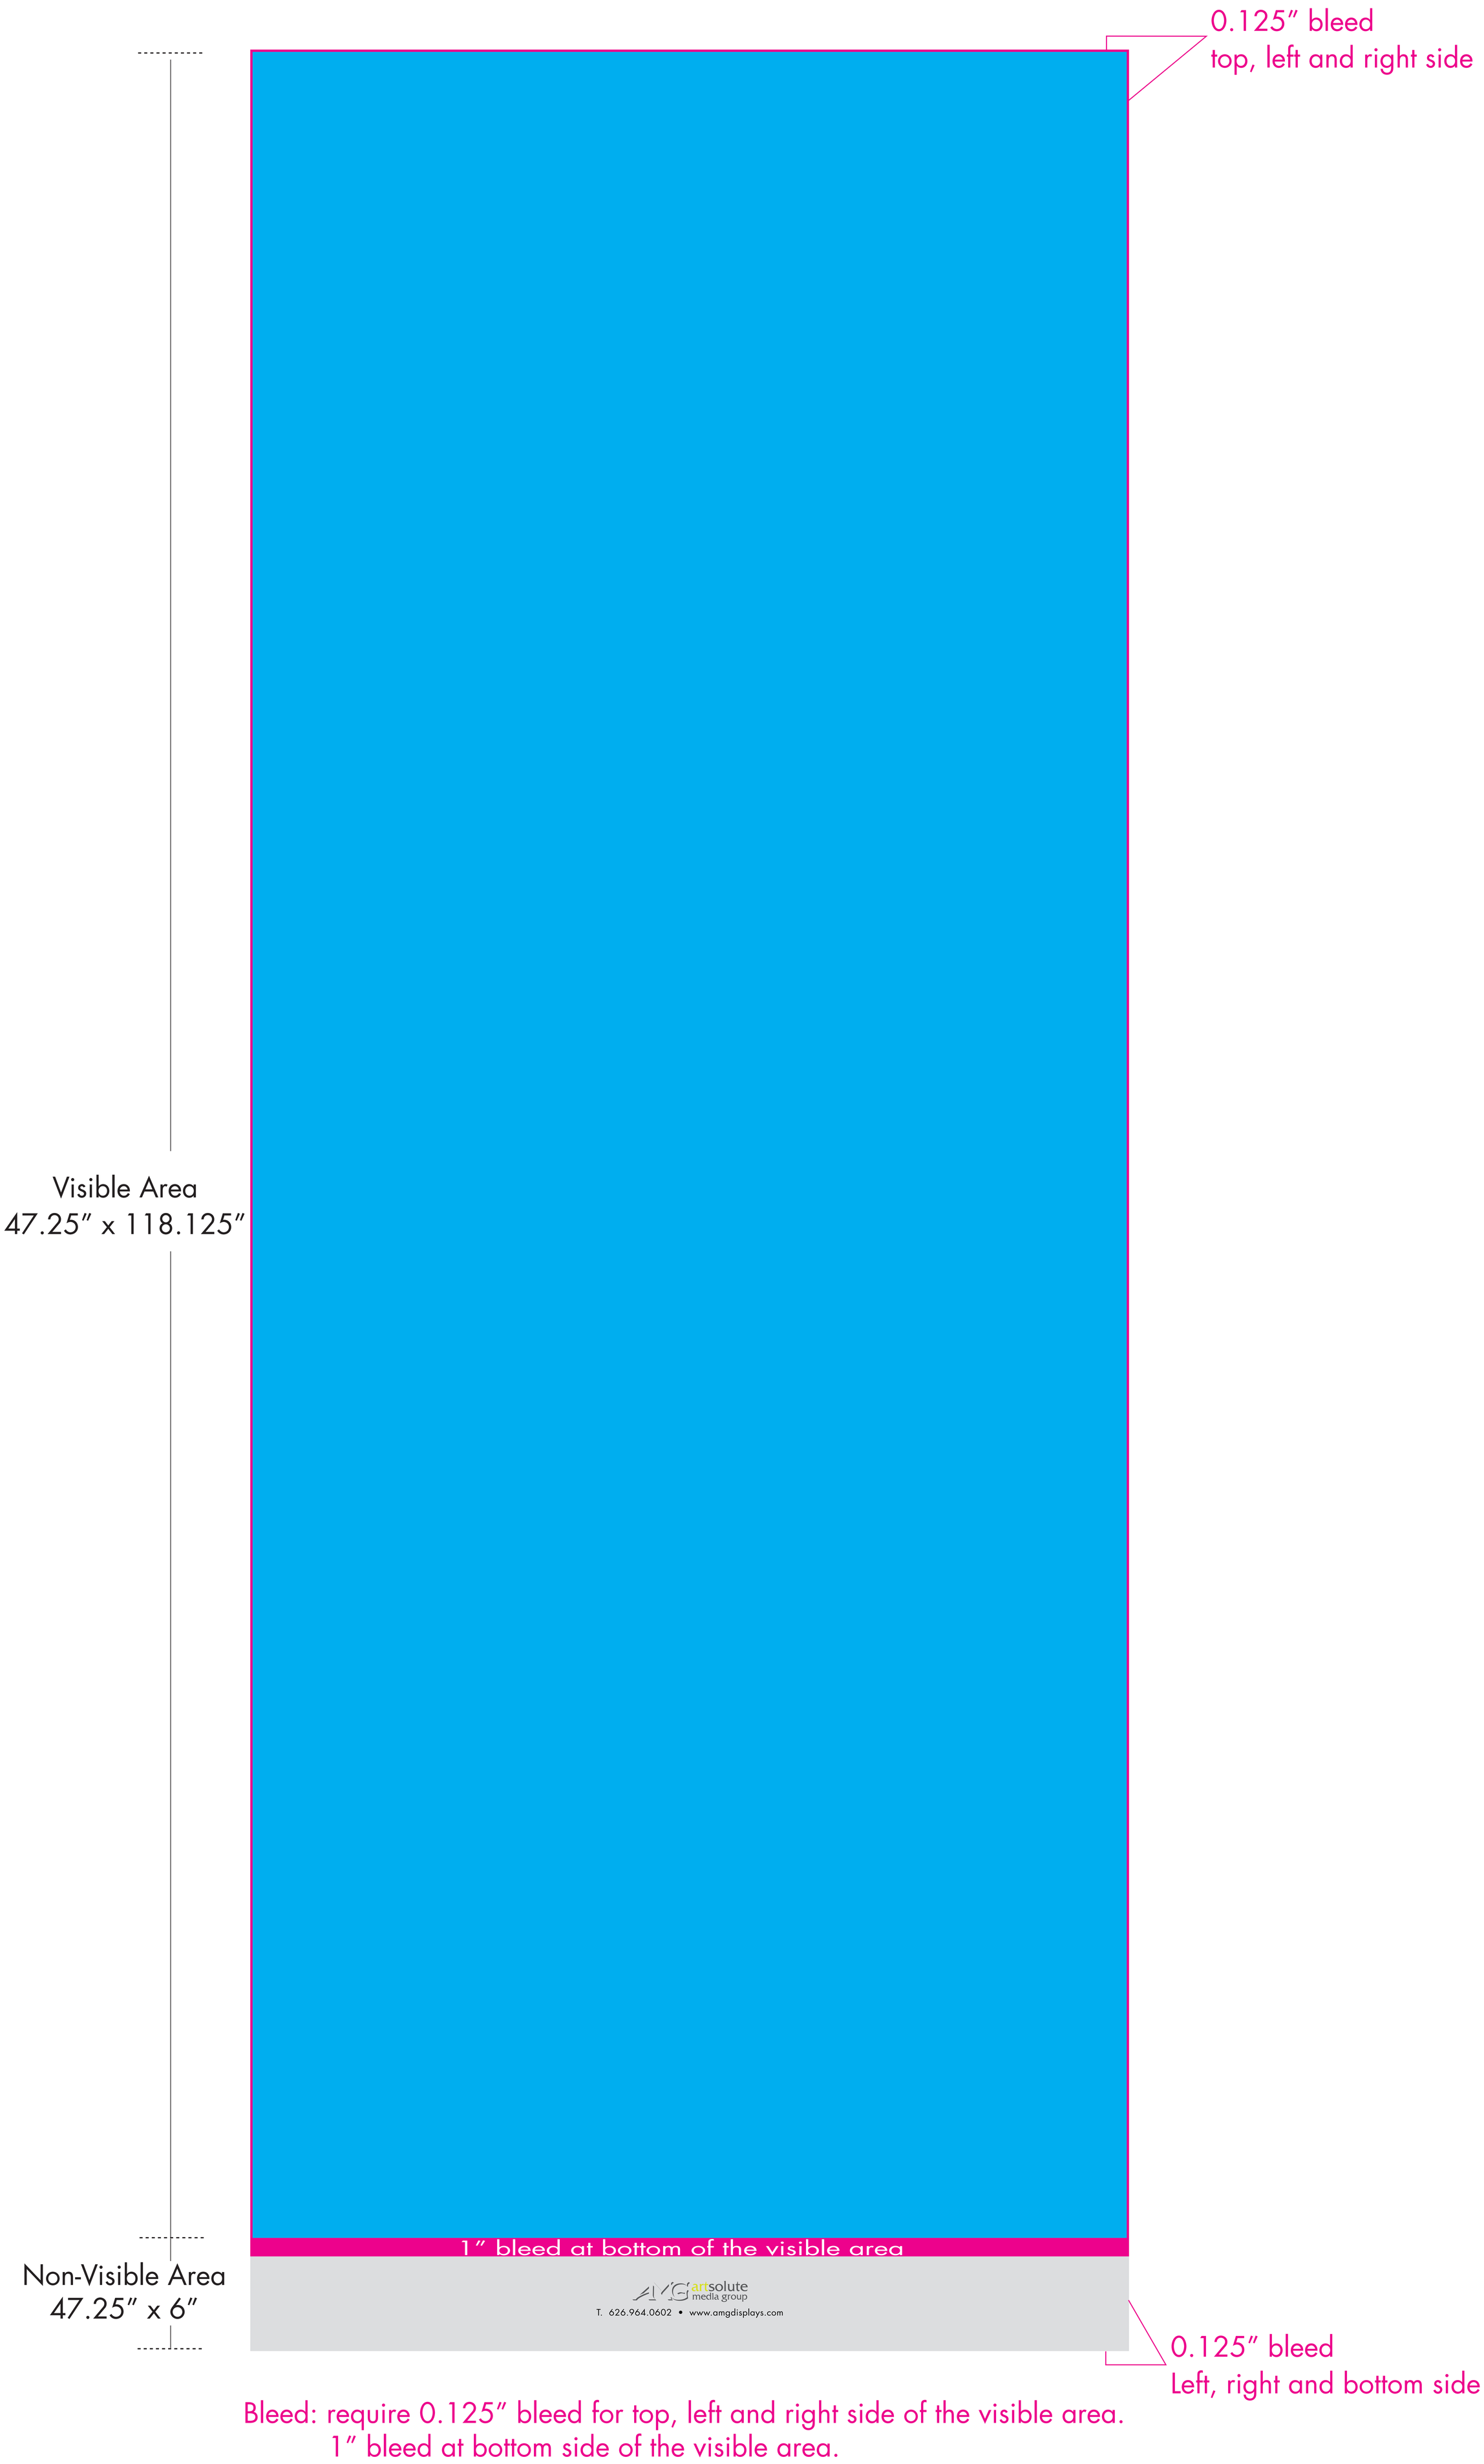

Bleed: require 0.125″ bleed for top, left and right side of the visible area.
1″ bleed at bottom side of the visible area.